

IV. NOTES ON USE

1. Use mild detergents for cleaning and disinfection. Do not use corrosive or abrasive products!
NOTE: Do not use agents containing naphtha, solvents, acids, chlorine etc. for cleaning soft surfaces!
2. Product marking is performed in the form of an identification label attached to each device. The label contains the following information:
 - number indicating the date of manufacture:
 - LOT: RRRR-MM (RRRR means the year, MM means the month, e.g.: 2023-01)
 - name and type of product REF: 12/MR
 - allowed body weight of the user
3. **All devices (except for caps) have a 2-year warranty.**
4. **Use the devices as directed!** Any bending of the metal parts with visible cracks on the surface exclude the device from further use.
Check the device before and during use to ensure that it has no scratches, cracks, etc.
5. The production service during the warranty period (24 months) includes replacement of parts or products, which are found to have any manufacturing defects.
6. The MIKIRAD operational service functions directly at the points of sale of the products.
7. MIKIRAD guarantees the production of spare parts for 10 years from the date of manufacture of a product.



INSTRUCTIONS FOR USE WALKING CANES

MIKIRAD manufactures **walking canes** as medical devices for improving the mobility of people with disabilities (according to In-house Specification ZN-00/MK-01-1/2006 harmonised with standard PN-EN ISO 9999 – Class 12 03 and EUROPEAN COUNCIL DIRECTIVE 2017/745 [MDR] of 5 April 2017)

PN EN ISO 9999	NAME	TYPE
12 03 03	Walking canes: - non-folding - folding canes	-10/MR, 11/MR, 12/MR; -14/MR;

I. BACKGROUND

Standard products are designed for users (with lower limb disability or prostheses) with height of 155cm to 185cm and body weight of up to 120 kg.

Each product is adapted to the user's height by moving the interconnected telescopic rods to obtain the desired height, and then locking them. This is done by stepwise adjustment (sliding the adjustment rods from the shaft in increments of 20 mm and locking them with a latch fitted to the holes in the rods or in the case of folding canes with a button.)

The height of a product is considered correct when the user has an upright posture when using the product, and the products works vertically, i.e. in the plane parallel to the body axis.

II. PROCEDURE FOR STEPWISE ADJUSTMENT OF PRODUCT HEIGHT (Fig. 2)

1. Push the double latch out of the holes by pushing both fronts of the latch wings towards the back using two thumbs, so as to move the wings and slide the steel pegs out of the rod holes.
Do not bend the latch wings as they may break or lose elasticity.
2. Slide the adjustment rod along the axis to the appropriate height for the user; remember that the holes in the adjustment rod must ideally overlap the holes in the shaft.
3. Insert the steel pegs of the latch into the correctly positioned holes and push the lath using your hand until the inside surface of the latch is in full contact with the rod shaft.

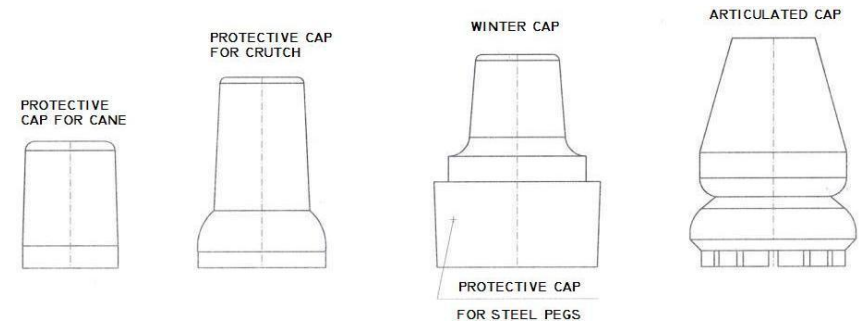


Fig.1 Protective cap

III. PROCEDURE FOR STEPWISE ADJUSTMENT OF PRODUCT HEIGHT WITH BUTTON (Fig. 3)

1. Press the button in.
2. Push the leg as if to shorten.
3. Turn the leg slightly.
4. Extend the leg to the required position, turn and re-locate button into the appropriate hole.
5. Check pins are fully located before use.

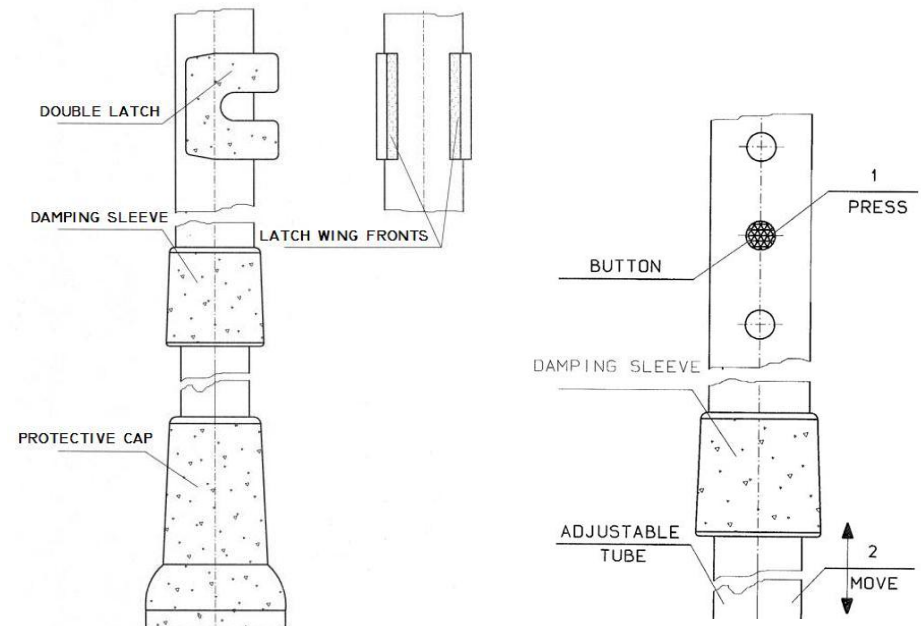
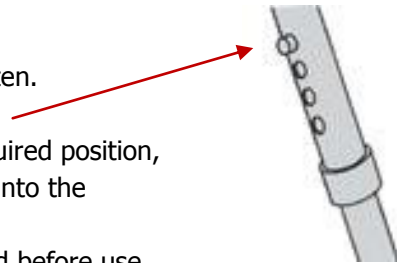


Fig.2 Stepwise adjustment

Fig.3 Stepwise adjustment with button

In winter, use an anti-slip winter cap, which is universal.